


Overview


Usage time	AHI	Leakage	Pressure
6:11 h	0 /h	40 %	6 hPa
The values displayed refer to days when the device was used (30 of 30).			

My therapy device			
Device:	prisma SMART	softPAP level:	soft0
Version:	3.7.0012	Therapy pressure:	min 4 hPa
Mode:	APAP		max 16 hPa


Usage time

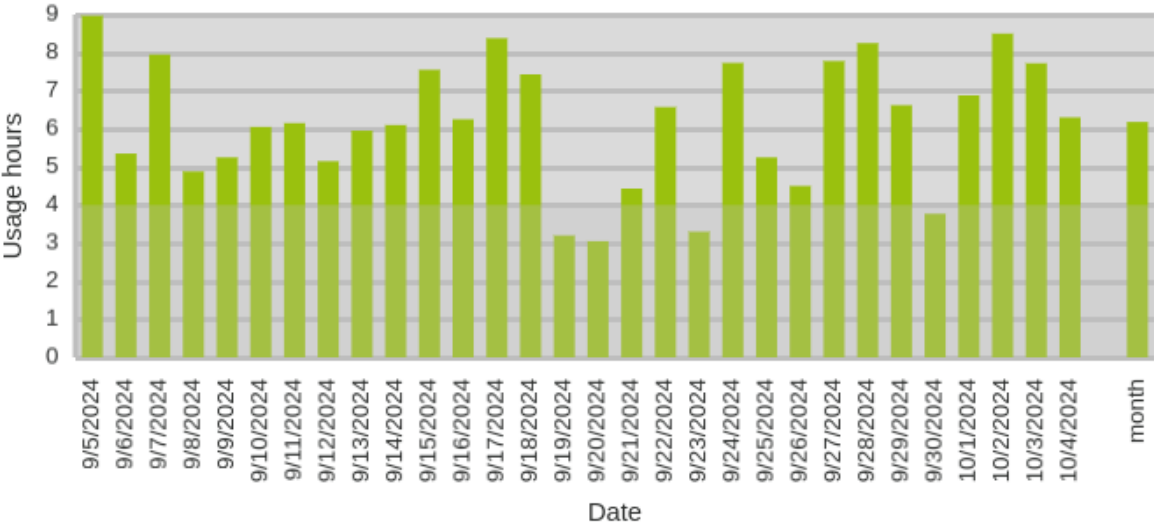


AHI

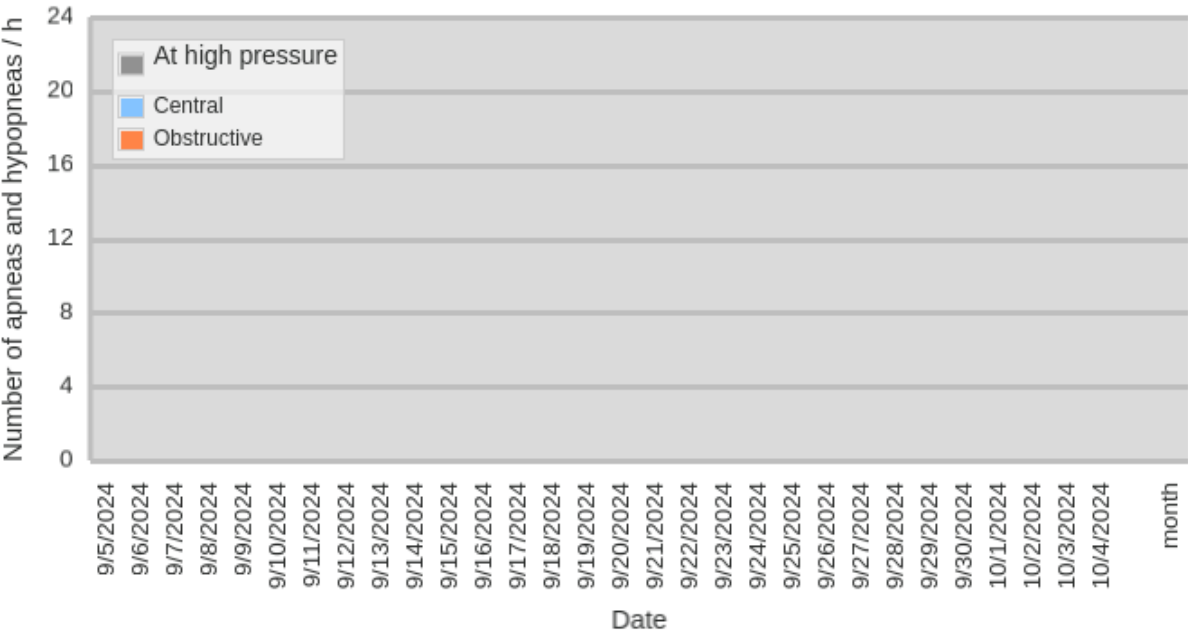

Deep sleep indicator

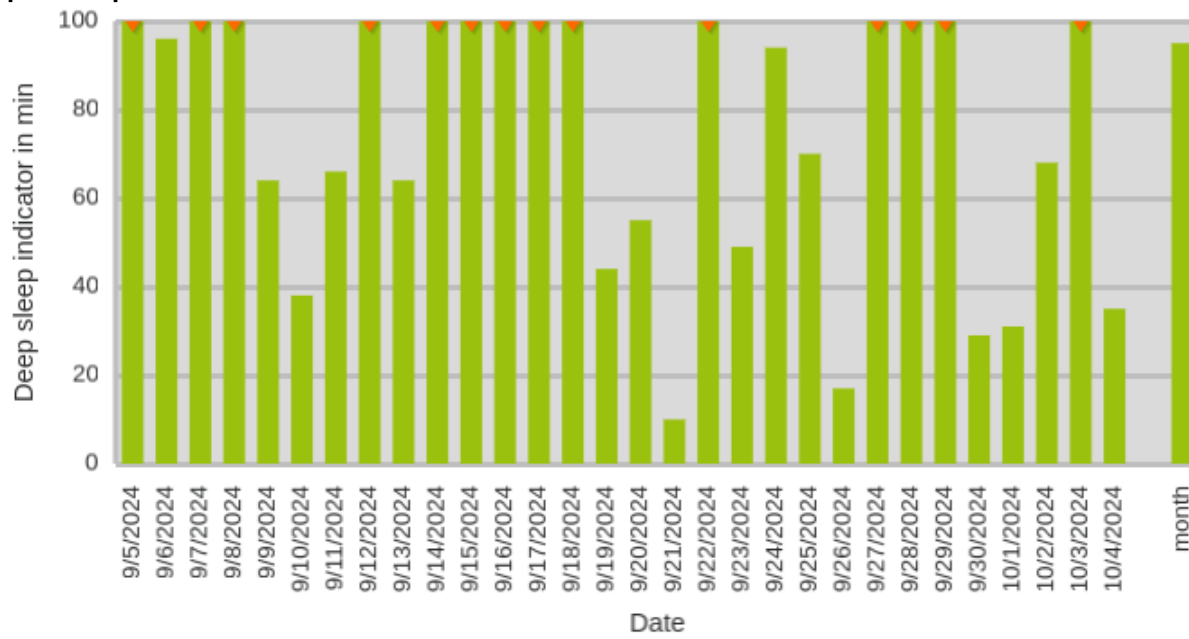

Pressure

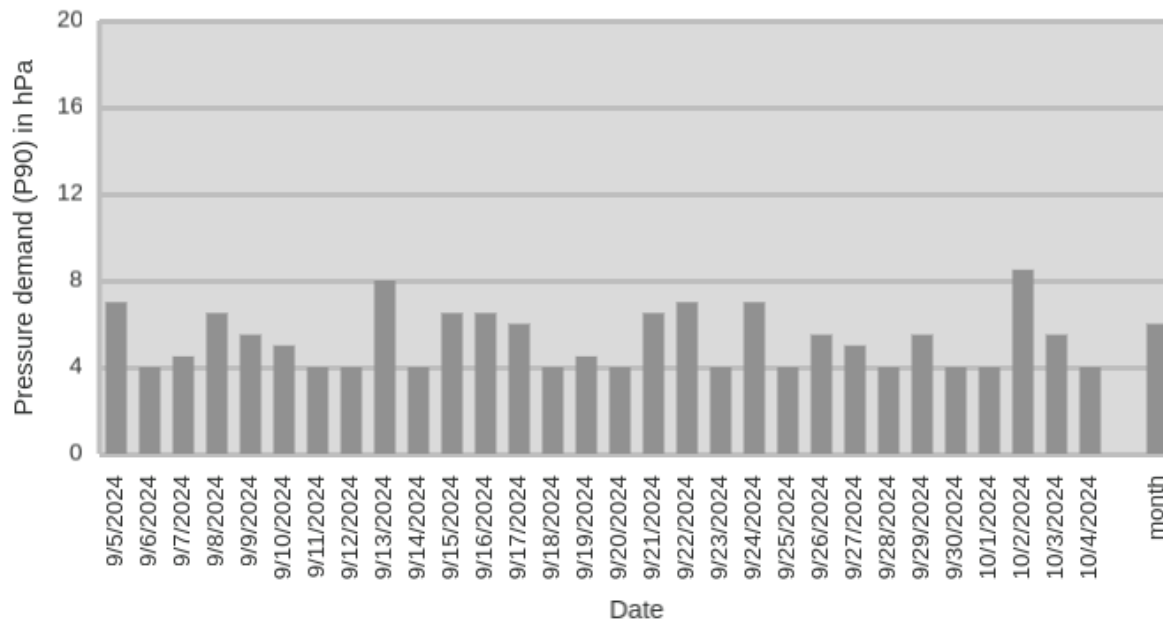

Leakage

